Ashton Coal

Monthly attended noise monitoring December 2021

Prepared for Ashton Coal Operations Pty Ltd January 2022





Servicing projects throughout Australia and internationally

SYDNEY

Ground floor, 20 Chandos Street St Leonards NSW 2065 T 02 9493 9500

NEWCASTLE

Level 1, 146 Hunter Street Newcastle NSW 2300 T 02 4907 4800

BRISBANE

Level 10, 87 Wickham Terrace Spring Hill QLD 4000 T 07 3648 1200

ADELAIDE

Level 1, 70 Pirie Street Adelaide SA 5000 T 08 8232 2253

MELBOURNE

187 Coventry Street South Melbourne VIC 3205

PERTH

PO Box 8155 Fremantle WA 6160

CANBERRA

PO Box 9148 Deakin ACT 2600

Ashton Coal

Monthly attended noise monitoring - December 2021

Report Number

H200894 RP12

Client

Ashton Coal Operations Pty Ltd

Date

4 January 2022

Version

v2 Final

Prepared by

Approved by

Lucas Adamson Senior Acoustic Consultant 4 January 2022

Hbb

Alex Dundon Associate 4 January 2022

This report has been prepared in accordance with the brief provided by the client and has relied upon the information collect ed at the time and under the conditions specified in the report. All findings, conclusions or recommendations contained in the report are based on the aforementioned circumstances. The report is for the use of the client and no responsibility will be taken for its use by other parties. The client may, at its discretion, use the report to inform regulators and the public.

© Reproduction of this report for educational or other non-commercial purposes is authorised without prior written permission from EMM provided the source is fully acknowledged. Reproduction of this report for resale or other commercial purposes is prohibited without EMM's prior written permission.

Table of Contents

1	Introduction					
2	Glossary of acoustic terms					
3	Noise	limits	4			
	3.1	Operational and sleep disturbance noise limits	4			
	3.2	Cumulative noise criteria	5			
	3.3	Low frequency noise criteria	5			
4	Asses	sment methodology	7			
	4.1	Attended noise monitoring	7			
	4.2	Instrumentation	7			
	4.3	Attended noise monitoring exceedance procedure	9			
	4.4	Determination of stability category	9			
5	Revie	w of data and discussion	11			
	5.1	Summary	11			
	5.2	N2 - Camberwell Village (west)	13			
	5.3	N3 - Camberwell Village (north east)	14			
	5.4	N4 - South of New England Highway	15			
6	Concl	usion	16			
Refe	erences		17			

Appendices

Appendix A	Project approval extract
Appendix B	EPL extract
Appendix C	Calibration certificates

Tables

Table 2.1	Glossary of acoustic terms	2
Table 2.2	Perceived change in noise	3
Table 3.1	Noise impact assessment criteria	4
Table 3.2	One-third octave low-frequency noise thresholds	6
Table 4.1	Attended noise monitoring locations	7
Table 4.2	Stability categories and temperature lapse rates	10
Table 5.1	Ashton Coal attended noise monitoring results – December 2021	12

Figures

Figure 2.1	Common noise levels	3
Figure 4.1	Noise monitoring locations and Ashton colliery boundary	8
Figure 5.1	N2 total measured one-third octave band frequencies	13
Figure 5.2	N3 total measured one-third octave band frequencies	14
Figure 5.3	N4 total measured one-third octave band frequencies	15

1 Introduction

EMM Consulting Pty Limited (EMM) was engaged to complete monthly attended noise surveys on behalf of Ashton Coal Operations Pty Ltd (Ashton Coal).

The purpose of the monitoring was to address requirements of the approved Ashton Coal Noise Management Plan (NMP), prepared to satisfy the requirements of the Development Consent DA 309-11-2001-I (DC) and Environment Protection License (EPL) 11879.

This report presents the results and findings of attended noise monitoring conducted on 20 December 2021.

The following material was referenced as part of this assessment:

- Department of Planning, Industry and Environment (DPIE), Development Consent 309-11-2001-I, as modified on 20 June 2016 (current as of 20 December 2021);
- Environment Protection Authority (EPA), Environment Protection License 11879, as varied on 3 February 2020 (current as of 20 December 2021);
- Ashton Coal Project Noise Management Plan (NMP), approved by DPIE on 23 September 2020 (current as of 27 October 2021);
- NSW EPA, Industrial Noise Policy (INP), 2000;
- NSW EPA, Industrial Noise Policy Application notes, 2017; and
- NSW EPA, Noise Policy for Industry (NPfI), 2017.

2 Glossary of acoustic terms

Several technical terms are discussed in this report. These are explained in Table 2.1.


Term	Description
dB	Noise is measured in units called decibels (dB). There are several scales for describing noise, the most common being the 'A-weighted' scale. This attempts to closely approximate the frequency response of the human ear.
L _{A1}	The 'A-weighted' noise level which is exceeded 1% of the time.
L _{A1,1 minute}	The 'A-weighted' noise level exceeded for 1% of the specified time period of 1 minute.
L _{A10}	The 'A-weighted' noise level which is exceeded 10% of the time. It is approximately equivalent to the average of maximum noise level.
L _{A90}	Commonly referred to as the background noise level. The 'A-weighted' noise level exceeded 90% of the time.
L _{Aeq}	The energy average noise from a source. This is the equivalent continuous 'A-weighted' sound pressure level over a given period. The L _{Aeq,15 minute} descriptor refers to an L _{Aeq} noise level measured over a 15-minute period.
L _{Amin}	The minimum 'A-weighted' noise level received during a measuring interval.
L _{Amax}	The maximum root mean squared 'A-weighted' sound pressure level (or maximum noise level) received during a measuring interval.
L _{Ceq}	The equivalent continuous 'C-weighted' sound pressure level over a given period. The L _{Ceq,15 minute} descriptor refers to an L _{Ceq} noise level measured over a 15 minute period. C-weighting can be used to measure low frequency noise.
Day period	Monday – Saturday: 7 am to 6 pm, on Sundays and Public Holidays: 8 am to 6 pm.
Evening period	Monday – Saturday: 6 pm to 10 pm, on Sundays and Public Holidays: 6 pm to 10 pm.
Night period	Monday – Saturday: 10 pm to 7 am, on Sundays and Public Holidays: 10 pm to 8 am.
Temperature inversion	A meteorological condition where the atmospheric temperature increases with altitude.

Table 2.1Glossary of acoustic terms

It is useful to have an appreciation of decibels (dB), the unit of noise measurement. Table 2.2 gives an indication as to what an average person perceives about changes in noise levels. Examples of common noise levels are provided in Figure 2.1.

Table 2.2Perceived change in noise

Change in sound pressure level (dB)	Perceived change in noise in surrounding environment
up to 2	not perceptible
3	just perceptible
5	noticeable difference
10	twice (or half) as loud
15	large change
20	four times (or quarter) as loud

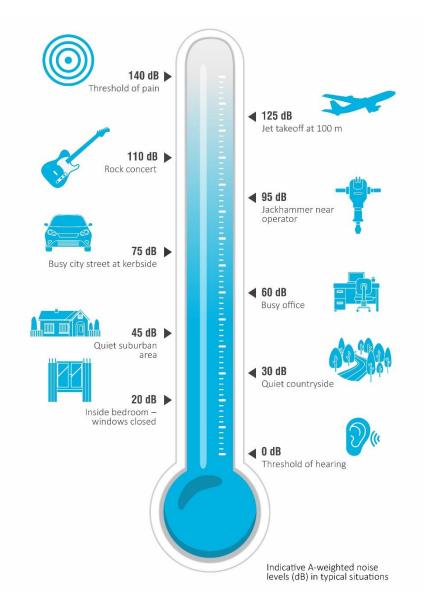



3 Noise limits

3.1 Operational and sleep disturbance noise limits

Ashton Coal noise limits are provided in Table 1, Condition 2 of Appendix 6 of the DC and Condition L4.1 of the EPL. Extracts of the relevant sections of the DC and EPL pertaining to noise are provided in Appendix A and B, respectively. The approved NMP adopts three attended noise monitoring locations that are representative of residences outlined in the DC. The noise monitoring locations and relevant criteria are summarised in Table 3.1.

Table 3.1 Noise impact assessment criteria

Monitoring location	Day	Day Evening		Night
	L _{Aeq,15 minute} , dB	L _{Aeq,15 minute} , dB	L _{Aeq,15 minute} , dB	L _{A1,1 minute} , dB
N2	38	38	36	46
N3	38	38	36	46
N4	38	38	36	46

The DC and the EPL specify the following meteorological conditions under which noise limits do not apply:

- during periods of rain or hail;
- average wind speed at microphone height exceeds 5 metres per second (m/s);
- wind speeds greater than 3 m/s at 10 metres above ground level; and
- temperature inversion conditions greater than 3°C/100m.

For this assessment, the recorded L_{Amax} has been used as a conservative estimate of the $L_{A1,1 \text{ minute}}$. The INP application notes state that the EPA accepts sleep disturbance analysis based on either the $L_{A1,1 \text{ minute}}$ or L_{Amax} metrics (EPA 2013), with use of L_{Amax} resulting in a more conservative assessment.

The DC and EPL state that modification factor corrections in the application notes to the INP (2017) shall be applied to the measured mine noise levels where applicable. The application notes to the INP state that Fact Sheet C of the NPfl (EPA 2017) now applies regarding the application of modifying factors.

3.2 Cumulative noise criteria

Ashton Coal cumulative noise limits are provided in Condition 5 and Condition 6 of Schedule 3 of the DC. An extract of the conditions relevant to cumulative noise criteria is provided here.

5. The Applicant must implement all reasonable and feasible measures to ensure that the noise generated by the Ashton Mine Complex combined with the noise generated by other mines in the vicinity does not exceed the criteria in Table 4 at any residence on any privately-owned land or on more than 25 per cent of any privately-owned land (except for the noise affected residential receivers in Table 1).

Table 4: Cumulative Noise Criteria dB(A) LAeq (period)

Location	Day	Evening	Night
Camberwell Village	55	45	40
All other privately-owned land	50	45	40

Cumulative noise is to be measured in accordance with the relevant requirements of the NSW Industrial Noise Policy. Appendix 8 sets out the requirements for evaluating compliance with these criteria.

6. If the cumulative noise generated by the Ashton Mine Complex combined with the noise generated by other coal mines in the vicinity exceeds the criteria in Table 5 at any residence on privately-owned land or more than 25 per cent of any privately-owned land (except for the noise-affected residential receivers ion Table 1), then upon receiving a written request from the landowner, the Applicant must, together with the relevant mines, acquire the land on as equitable basis as possible, in accordance with the procedures in conditions 7 and 8 of schedule 4.

Table 5: Cumulative Noise Acquisition Criteria dB(A) LAeq (period)

Location	Day	Evening	Night
Camberwell Village	60	50	45
All other privately-owned land	55	50	45

Cumulative noise is to be measured in accordance with the relevant requirements of the NSW Industrial Noise Policy. Appendix 8 sets out the requirements for evaluating compliance with these criteria.

3.3 Low frequency noise criteria

Condition 3 of Appendix 8 of the DC states that noise generated by Ashton Coal is to be measured in accordance with the relevant requirements of the INP. The INP application notes state that Section 4 of the INP has been withdrawn and the modifying factor adjustments outlined in Fact Sheet C of the NPfI are to be used when assessing the characteristics of a noise source.

Fact sheet C of the NPfI (EPA 2017) provides guidelines for applying modifying factor corrections to account for low frequency noise emissions. The NPfI specifies that a difference of 15 dB or more between site 'C-weighted' and site 'A-weighted' noise emission levels identifies the potential for an unbalanced spectrum and potential increased annoyance.

Where a difference of 15 dB or more between site 'C-weighted' and site 'A-weighted' noise emission levels is identified, the one-third octave noise levels recorded should be compared to the values in Table C2 of the NPfI (EPA 2017), which has been reproduced in Table 3.2 below.

Table 3.2 One-third octave low-frequency noise thresholds

One-third octave Lzeq,15 minute threshold level													
Frequency (Hz)	10	12.5	16	20	25	31.5	40	50	63	80	100	125	160
dB (Z)	92	89	86	77	69	61	54	50	50	48	48	46	44

The following modifying factor correction is to be applied where the site 'C-weighted' and site 'A-weighted' noise emission level is 15 dB or more and:

- where any of the one-third octave noise levels in Table 3.2 are exceeded by up to and including 5 dB and cannot be mitigated, a 2 dB positive adjustment to measured/predicted A-weighted levels applies for the evening/night period; or
- where any of the one-third octave noise levels in Table 3.2 are exceeded by more than 5 dB and cannot be mitigated, a 5 dB positive adjustment to measured/predicted A-weighted levels applies for the evening/night period.

Hence, where relevant throughout each survey the operator has estimated the difference between site 'C-weighted' and site 'A-weighted' noise emission levels by matching audible sounds with the response of the analyser $(L_{Ceq}-L_{Aeq})$. Where this was deemed to be 15 dB or greater, the measured one-third octave frequencies have been compared to the values in Table 3.2 to identify the relevant modifying factor correction (if applicable). This method has been applied to this assessment as presented in Section 5.

It is of note that the NPfI (EPA 2017) states that low-frequency noise corrections only apply under the standard or noise-enhancing meteorological conditions.

4 Assessment methodology

4.1 Attended noise monitoring

To quantify noise emissions from Ashton Coal, 15-minute attended noise monitoring surveys were completed at representative locations as per the approved NMP. Noise monitoring locations and their coordinates are listed in Table 4.1 and are shown in Figure 4.1.

Table 4.1 Attended noise monitoring locations


Monitoring location	Description	MGA56		
		Easting	Northing	
N2	Camberwell Village (west)	320297	6405670	
N3	Camberwell Village (north east)	320554	6405839	
N4	South of New England Highway	319776	6404101	

Attended noise monitoring is scheduled to be "unannounced" and, to EMM's knowledge, Ashton Coal were not aware of the monitoring prior to its commencing. Noise monitoring is avoided during any scheduled downtime or major maintenance. Information provided by Ashton Coal after completion of the noise monitoring confirmed that regular operations were occurring during the monitoring period.

Where possible throughout each survey, the operator has quantified the contribution of each significant noise source. This was done by matching audible sounds with the response of the analyser (where applicable) and/or via post-analysis of data (eg low pass filtering).

4.2 Instrumentation

A Brüel & Kjær 2250 Type 1 sound analyser (s/n 3008201) was used to conduct 15-minute attended measurements and record 1/3 octave frequency and statistical noise indices. The sound analyser was calibrated before and on completion of the survey using a Svantek SV-36 calibrator (s/n 79952). The instrumentation's calibration certificates are provided in Appendix C.

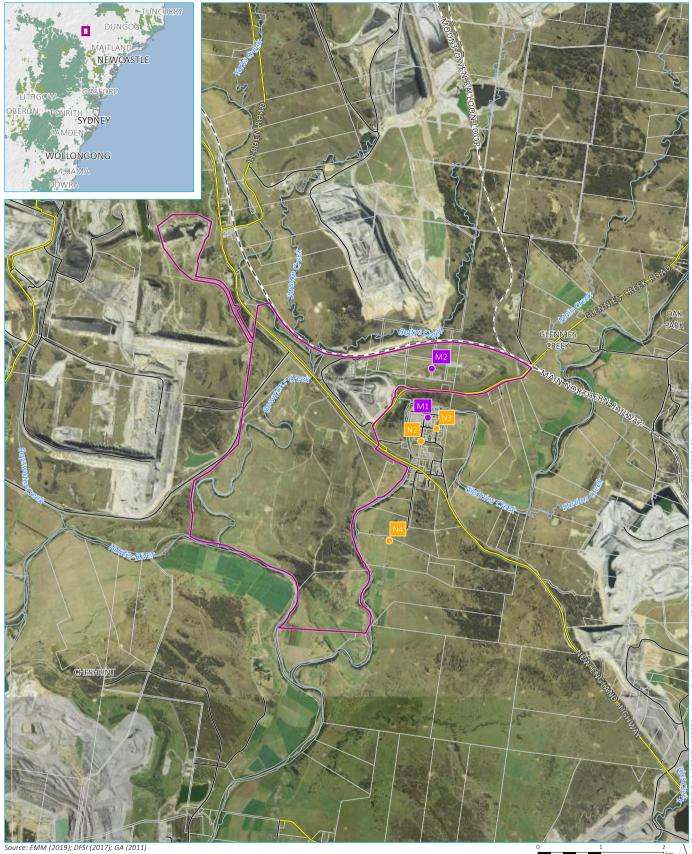

KEY

- Site boundary
- Noise monitoring location
- Meteorological station
- – Rail line
 Main road
- ---- Local road
- Cadastral boundary

GDA 1994 MGA Zone 56 N

Noise monitoring locations and Ashton colliery boundary

Ashton Coal Monthly attended noise monitoring Figure 4.1



4.3 Attended noise monitoring exceedance procedure

Ashton Coal has developed an attended monitoring exceedance procedure that is to be implemented if measurements show Ashton Coal noise emissions are above the relevant noise criteria. This response plan is implemented if site noise levels are determined to be above the relevant noise criteria and when noise limits are applicable due to suitable meteorological conditions. The following noise management initiatives are implemented:

- Consultant will record the reading and advise Ashton Coal of the exceedance. Ashton Coal will implement remedial action as required.
- A follow up measurement is to be conducted (within 75 minutes after the first measurement and no earlier than 10 pm).
- If the follow up measurement indicates that site noise levels are above the relevant noise criteria and that noise limits are applicable, the consultant will record the result, note the site has failed and is deemed a 'noise affected night' at that location. An additional monitoring test should be scheduled to be undertaken at the same location within one week and move on to the next monitoring location.
- If the follow up measurement indicates that site noise levels are below the relevant noise criteria and that noise limits are applicable, the consultant will record the result, note the site has passed, schedule an additional monitoring test to be undertaken at the location within one week and move on to the next monitoring location.

4.4 Determination of stability category

As per Condition L4.4, this assessment determined the stability categories throughout the attended monitoring period using the direct measurement method as per Appendix E2 of the INP (EPA 2000).

The temperature lapse rate between the two weather stations (M1 – Sentinex Unit 40 located in Camberwell Village and M2 – Ashton Coal 'repeater' meteorological station located in the north eastern open cut (NEOC) area) was calculated using the following formula:

Temperature lapse rate =
$$(\Delta T) \times (100/(\Delta H))$$

Where:

- ΔT = temperature measured at M2 (at 10 metres above ground level) minus temperature measured at M1 (at 10 metres above ground level); and
- ΔH = the vertical height difference between M2 and M1 (equal to 73 metres).

Table E1 of the INP (EPA 2000) is reproduced in Table 4.2 and presents the stability categories and associated ranges in temperature lapse rates.

Table 4.2 Stability categories and temperature lapse rates

Stability category	Temperature lapse rate (ΔT) (°C/100 m)	
A	ΔT < -1.9	
В	-1.9 ≤ ΔT < -1.7	
C	-1.7 ≤ ΔT < -1.5	
D	-1.5 ≤ ΔT < -0.5	
E	-0.5 ≤ ΔT < 1.5	
F	$1.5 \le \Delta T < 4.0$	
G	$\Delta T \ge 4.0$	

Source: INP (EPA 2000).

Other meteorological data, such as wind speed, has been sourced directly from meteorological station M2 since it is more representative of the weather conditions nearer to the Ashton Coal noise sources.

5 Review of data and discussion

5.1 Summary

Results of attended noise measurements are summarised in Table 5.1. Ashton Coal contribution and total mine noise were determined for each survey using in-field observations and post-analysis of data as required (eg removing higher frequencies that are not mine related, ie above 630 Hz). Attended monitoring was completed on 20 December 2021. Noise from Ashton Coal operations was audible during all three operator-attended noise surveys.

The meteorological data for the monitoring period was sourced from Ashton Coal's two weather stations (M1 and M2) to determine applicability of criteria in accordance with the DC and EPL. Noise limits were found to be applicable during all three measurements.

Low frequency noise was initially conservatively assessed by comparison of the total measured one-third octave L_{Aeq} noise levels to the NPfI one-third octave low-frequency noise thresholds. Total measured LFN thresholds were exceeded during the measurement at N2 and therefore a more detailed analysis of overall mining noise contributions was conducted. The surveys were reviewed for periods with low levels of extraneous noise (such as traffic and other mines in the area) as to determine and assess the Ashton Coal low-frequency noise contributions to the total LFN levels. It was determined that the relevant LFN thresholds would not have been exceeded solely by noise emissions from Ashton Coal due to the following:

- the relative contribution of Ashton Coal (31 dB L_{Aeq,15 minute});
- the relative contribution of other mines in the area (35 dB L_{Aeq,15 minute});
- the relative contribution from traffic on the New England Highway (consistent and dominant at times);
- the level/nature of the exceedance of the relevant LFN threshold (2 dB exceedance at 500 Hz); and
- onsite operations were relatively consistent during the measurement (ie fixed and mobile plant activities).

Therefore, in accordance with the NPfI, an LFN modifying factor was not applied to estimated Ashton Coal noise levels at N2.

Notwithstanding the preceding, it is noted that total measured noise levels exceeded the relevant LFN thresholds during the measurement at N2 and therefore, in accordance with the NPfI, an LFN modifying factor was applied to the estimated cumulative mine noise level at location N2.

Ashton Coal noise contributions and cumulative mine noise contributions were below (ie complied with) the relevant noise limits at all monitoring locations.

					Total r	noise leve	els, dB			Site con	tributio	ns, dB	Noise li	imits, dB	Meteorological	Exceedance	Comments
Location	Date	Start time	L _{Amin}	L _{A90}	L _{Aeq}	L _{A10}	L _{A1}	L _{Amax}	L _{Ceq}	LFN mod. factor ¹	L _{Aeq}	L _{Amax} ²	L _{Aeq}	L _{Amax} ²	conditions ³ limits apply (Y/N)	dB	
N2	20/12	22:08	36	38	45	49	53	59	60	Nil	31	32	36	46	1.5 m/s @ 173° E class stability 0.7°C/100m VTG Y	Nil	Ashton Coal mine hum consistently audible. Other mines in the vicinity (35 dB L _{Aeq,15 minute}), insects, frogs and traffic on the New England Highway consistently audible. Bird noise, livestock and resident noise occasionally audible.
N3	20/12	22:27	34	36	41	44	50	53	58	Nil	29	31	36	46	1.8 m/s @ 157° E class stability 1.1°C/100m VTG Y	Nil	Ashton Coal mine hum consistently audible. Other mines in the vicinity (35 dB L _{Aeq,15 minute}), traffic on the New England Highway, insects and frogs consistently audible. Dogs barking occasionally audible.
N4	20/12	22:50	31	33	36	39	43	47	57	Nil	IA	IA	36	46	1.4 m/s @ 145° F class stability 1.6°C/100m VTG Y	Nil	Ashton Coal inaudible. Other mines in the vicinity (31 dB L _{Aeq,15 minute}) occasionally audible. Traffic on the New England Highway, insects and frogs consistently audible.

Table 5.1 Ashton Coal attended noise monitoring results – December 2021

Notes: 1. Modifying factor correction for low frequency noise in accordance with Fact Sheet C of the NPfl (refer Section 3.3).

2. For assessment purposes the L_{Amax} and the $L_{\text{A1,1}\,\text{minute}}$ are interchangeable.

3. Meteorological data were taken as an average over 15 minutes from the Ashton Coal weather station (Refer to Section 5.1). VTG assumes the temperature sensors on the two weather stations are in proper working order and calibrated to manufacturers requirements.

4. IA = inaudible.

5. N/A = not applicable.

5.2 N2 - Camberwell Village (west)

Ashton Coal operations were consistently audible during the operator-attended noise survey including conveyor hum. The Ashton Coal mine noise contribution was estimated at up to 31 dB L_{Aeq,15 minute}. Conveyor hum from site generated an estimated 32 dB L_{Amax}. Ashton Coal noise contributions complied with the DC and EPL noise limits. Other ambient noise sources included other mines in the vicinity, insects, frogs, traffic on the New England Highway, bird noise, livestock and resident noise. A graph of the total linear noise levels measured in each one-third octave frequency bands is shown in Figure 5.1.

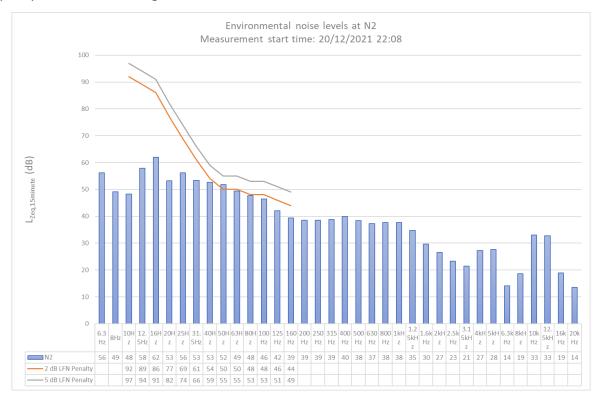


Figure 5.1 N2 total measured one-third octave band frequencies

Other mining operations in the vicinity were consistently audible during the operator-attended noise survey at monitoring location N2. The total cumulative mine noise contribution was estimated to be 35 dB $L_{Aeq,night}$ (ie Ashton Coal mine noise of 31 dB $L_{Aeq,15 minute}$ + Other mine noise of 35 dB $L_{Aeq,15 minute}$ - 3 dB + 2 dB as per NPfl methodology), including a 2 dB positive adjustment for LFN. This is below the cumulative mine noise night-time criterion (ie $L_{Aeq,night}$ 40 dB). Therefore, the total cumulative mine $L_{Aeq,night}$ noise contribution was below the cumulative mine noise criterion.

5.3 N3 - Camberwell Village (north east)

Ashton Coal operations were consistently audible during the operator-attended noise survey including conveyor hum. The Ashton Coal mine noise contribution was estimated at up to 29 dB L_{Aeq,15 minute}. Conveyor hum from site generated an estimated 31 dB L_{Amax}. Ashton Coal noise contributions complied with the DC and EPL noise limits. Other ambient noise sources included other mines in the vicinity, insects, frogs, traffic on the New England Highway and dogs barking. A graph of the total linear noise levels measured in the one-third octave frequency bands is shown in Figure 5.2.

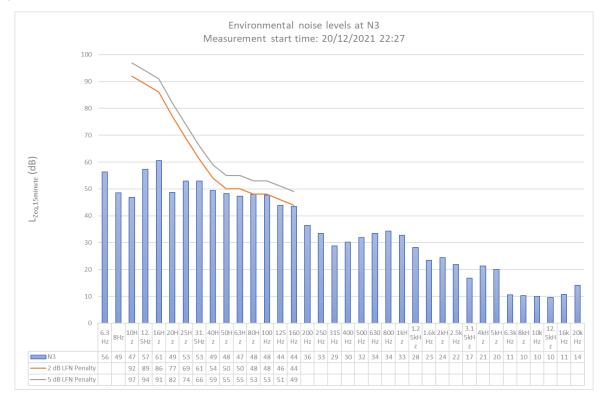


Figure 5.2 N3 total measured one-third octave band frequencies

Other mining operations in the vicinity were consistently audible during the operator-attended noise survey at monitoring location N3. The total cumulative mine noise contribution was estimated to be 33 dB $L_{Aeq,night}$ (ie Ashton Coal mine noise of 29 dB $L_{Aeq,15 minute}$ + Other mine noise of 35 dB $L_{Aeq,15 minute}$ - 3 dB as per NPfl methodology). This is below the cumulative mine noise night-time criterion (ie $L_{Aeq,night}$ 40 dB). Therefore, the total cumulative mine $L_{Aeq,night}$ noise contribution was below the cumulative mine noise criterion.

5.4 N4 - South of New England Highway

Ashton Coal operations were inaudible during the entire operator-attended noise survey. Given this and the measured background noise level of 33 dB L_{A90} , the Ashton Coal $L_{Aeq,15 \text{ minute}}$ mine noise contribution was estimated to be ≤ 23 dB $L_{Aeq,15 \text{ minute}}$ and therefore below the relevant noise limit. Ashton Coal noise contributions would have complied with the DC and EPL noise limits. Other ambient noise sources included other mines in the vicinity, insects, frogs and traffic on the New England Highway. A graph of the total linear noise levels measured in one-third octave frequency bands is shown below in Figure 5.3.

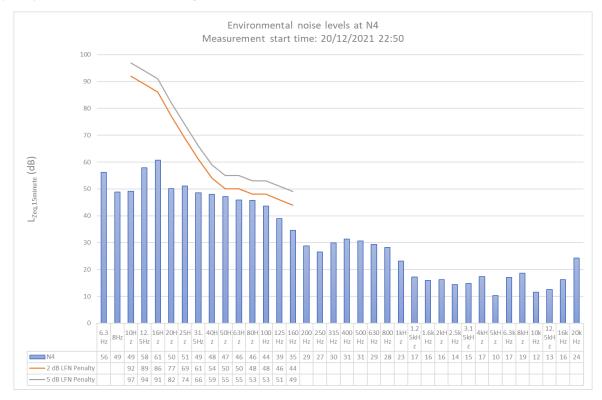


Figure 5.3 N4 total measured one-third octave band frequencies

Other mining operations in the vicinity were consistently audible during the operator-attended noise survey at monitoring location N4. The total cumulative mine noise contribution was estimated to be 28 dB $L_{Aeq,night}$ (ie other mine noise of 31 dB $L_{Aeq,15 minute}$ - 3 dB as per NPfI methodology). This is below the cumulative mine noise night-time criterion (ie $L_{Aeq,night}$ 40 dB). Therefore, the total cumulative mine $L_{Aeq,night}$ noise contribution was below the cumulative mine noise criterion.

6 Conclusion

EMM has completed a review of mine noise from Ashton Coal within the surrounding community based on attended measurements conducted on 20 December 2021.

The applicability of noise limits was assessed with reference to Ashton Coal's two meteorological stations (M1 and M2) located to the east of the site. Noise limits were found to be applicable during all three measurements.

The assessment of noise contributions from site included consideration of modifying factors for noise characteristics, where relevant, and in accordance with the DC and EPL.

Ashton Coal noise contributions and cumulative mine noise contributions were at or below (satisfied) the relevant noise limits at all monitoring locations for this round of monitoring.

References

Ashton Coal Noise Management Plan, 2017.

NSW Department of Planning, Industry and Environment, Development Consent DA309-11-2001-I, 2016. NSW Environment Protection Authority, Environment Protection License 11879. NSW Environment Protection Authority, Industrial Noise Policy, 2000. NSW Environment Protection Authority, Industrial Noise Policy Application notes, 2017. NSW Environment Protection Authority, Noise Policy for Industry, 2017. Appendix A

Project approval extract

APPENDIX 6 ALTERNATE NOISE CONDITIONS

NOISE

Application

1. Conditions 2 to 3 below have effect during times when open cut mining operations are not being undertaken at the Ashton Mine Complex, in the opinion of the Secretary.

Noise Criteria

 Except for the noise-affected land in Table 1 of Schedule 3, the Applicant must ensure that the noise generated by the development does not exceed the criteria in Table 1 at any residence on privatelyowned land or on more than 25 per cent of any privately-owned land.

Table 1: Noise	e Criteria dB(A)				
Receiver No.	Receiver	Day (L _{Aeg (15min)})	Evening (L _{Aeg (15min}))	Night (L _{Aeg (15min)})	Night (L _{A1 (1 min)})
-	All privately-owned land	38	38	36	46

Noise generated by the development is to be measured in accordance with the relevant requirements of the *NSW Industrial Noise Policy*. Appendix 8 sets out the requirements for evaluating compliance with these criteria.

However, these noise criteria do not apply if the Applicant has an agreement with the relevant owner/s of the residence/land to generate higher noise levels, and the Applicant has advised the Department in writing of the terms of this agreement.

Additional Noise Mitigation Measures

3. Upon receiving a written request from the owner of any residence on any privately-owned land where subsequent operational noise monitoring shows the noise generated by the development exceeds the noise limits in Table 2, the Applicant must implement additional reasonable and feasible noise mitigation measures (such as double glazing, insulation, and/or air conditioning) at the residence in consultation with the owner.

If within 3 months of receiving this request from the landowner, the Applicant and the landowner cannot agree on the measures to be implemented, or there is a dispute about the implementation of these measures, then either party may refer the matter to the Secretary for resolution.

Receiver	Receiver	Day	Evening	Night
No.		(L _{Aeg (15min)})	(L _{Aeg (15min)})	(L _{Aeg (15min)})
-	All privately-owned land	38	38	38

Table 2: Additional Noise Mitigation Criteria dB(A) LAeq (15min)

Notes:

- Noise generated by the development is to be measured in accordance with the relevant requirements of the NSW Industrial Noise Policy. Appendix 8 sets out the requirements for evaluating compliance with these criteria.
- For this condition to apply, the exceedance of the criteria must be systemic.

APPENDIX 8 NOISE COMPLIANCE ASSESSMENT

Compliance Monitoring

- 1. Attended monitoring is to be used to evaluate compliance with the relevant conditions of this approval.
- 2. Data collected for the purposes of determining compliance with the relevant conditions of this approval is to be excluded under the following meteorological conditions:
 - a) during periods of rain or hail;
 - b) average wind speed at microphone height exceeds 5 m/s;
 - c) wind speeds greater than 3 m/s measures at 10 m above ground level; and
 - d) temperature inversion conditions greater than 3°C/100m.
- 3. Unless otherwise agreed with the Secretary, this monitoring is to be carried out in accordance with the relevant requirements relating for reviewing performance set out in the NSW Industrial Noise Policy (as amended from time to time), in particular the requirements relating to:
 - a) monitoring locations for the collection of representative noise data;
 - b) equipment used to collect noise data, and conformity with Australian Standards relevant to such equipment; and
 - c) modifications to noise data collected, including for the exclusion of extraneous noise and/or penalties for modifying factors apart from adjustments for duration.
- 4. To the extent that there is any inconsistency between the Industrial Noise Policy and the requirements set out in this Appendix, the Appendix prevails to the extent of the inconsistency.

Determination of Meteorological Conditions

 Except for wind speed at microphone height, the data to be used for determining meteorological conditions shall be that recorded by the meteorological station located in the vicinity of the site (as required by condition 18 of Schedule 3). Appendix B



Environment Protection Licence

Licence - 11879



L3 Waste

- L3.1 The licensee must not cause, permit or allow any waste to be received at the premises unless specified in this licence.
- L3.2 The Licensee must not dispose of waste on the premises unless authorised by a condition of this Licence.

L4 Noise limits

L4.1 Noise from the premises must not exceed the noise limits specified in the table below.

Residences referenced in this table are from the consent DA 309-11-2001-i and summarised in the EPA reference DOC19/761196.

Location	Day LAeq(15 minute)	Evening LAeq(15 minute)	Night LAeq(15 minute)	Night LAeq(1 minute)
EPA Point 13	38	38	36	46
EPA Point 14	38	38	36	46
EPA Point 15	38	38	36	46
All other privately owned residences	38	38	36	46

L4.2 For the purpose of Condition L4.1:

a) Day is defined as the period from 7am to 6pm Monday to Saturday and 8am to 6pm Sundays and Public Holidays,

b) Evening is defined as the period from 6pm to 10pm, and

c) Night is defined as the period from 10pm to 7am Monday to Saturday and 10pm to 8am Sundays and Public Holidays

- L4.3 The noise emission limits identified in condition L4.1 apply under the following meteorological conditions:
 - a) wind speeds up to 3m/s at 10m above ground level; and
 - b) temperature inversion conditions up to 3 degrees C/100m.

L4.4 For the purposes of condition L4.1:

a) Data recorded by the closest and most representative meteorological station installed on the premises at EPA Identification Point 12 must be used to determine meteorological conditions; and

b) Temperature inversion conditions (stability category) are to be determined by the methods referred to

in Fact Sheet D of the Noise Policy for Industry (2017) using EPA Identification Points 12 and 32.

4 Operating Conditions

Appendix C Calibration certificates

CERTIFICATE OF CALIBRATION

B&K

2250

4189

CERTIFICATE NO.: SLM 26291 & FILT 5615

2759405

2888134

2759405

Jack Kiel

05/02/2020

Serial No:

Serial No:

Serial No:

Serial No: 16037

Equipment Description: Sound Level Meter

Manufacturer: Model No:

Microphone Type: Preamplifier Type:

ZC0032

1/3 Octave

Filter Type:

Comments:

Owner:

EMM Consulting Level 3, 175 Scott Street Newcastle, NSW 2300

(See over for details)

All tests passed for class 1.

Ambient Pressure:

1007 hPa ±1.5 hPa

Temperature:

24 °C ±2° C Relative Humidity: 53% ±5%

Issue Date:

Date of Calibration: 05/02/2020 Acu-Vib Test Procedure: AVP10 (SLM) & AVP06 (Filters)

CHECKED BY:

AUTHORISED SIGNATURE:

Accredited for compliance with ISO/IEC 17025 - Calibration The results of the tests, calibration and/or measurements included in this document are traceable to Australian/national standards.





HEAD OFFICE Unit 14, 22 Hudson Ave. Castle Hill NSW 2154 Tel: (02) 96808133 Fax: (02)96808233 Mobile: 0413 809806 web site: www.acu-vib.com.au

Accredited Lab. No. 9262 Acoustic and Vibration Measurements

Page 1 of 2 AVCERT10 Rev. 1.3 15.05.18

CERTIFICATE OF CALIBRATION

CERTIFICATE NO.: SLM 25410 & FILT 5368

Equipment Description: Sound Level Meter

Manufacturer:	B&K		
Model No:	2250	Serial No:	3008201
Microphone Type:	B&K 4189	Serial No:	2983733
Preamplifier Type:	B&K ZC0032	Serial No:	22666
Filter Type:	1/3 Octave	Serial No:	3008201
Comments:	All tests passe (See over for		
Owner:	EMM Consult Ground Floor, St Leonards N	ng Suite 01, 20	Chandos St
Ambient Pressure:	1002 hPa ±1	.5 hPa	
Temperature:	23 °C ±2° (C Relative Hu	midity: 29% ±5%
Date of Calibration: Acu-Vib Test Procedure	21/08/2019 :: AVP10 (SLM	Issue Date) & AVP06 (F	21/08/2019 ilters)

CHECKED BY: IRB

AUTHORISED SIGNATURE:

Hein Soe

Accredited for compliance with ISO/IEC 17025 - Calibration The results of the tests, calibration and/or measurements included in this document are traceable to Australian/national standards.





 HEAD OFFICE

 Unit 14, 22 Hudson Ave.
 Castle Hill NSW 2154

 Tel: (02) 96808133
 Fax: (02)96808233

 Mobile: 0413 809806
 web site: www.acu-vib.com.au

Accredited Lab. No. 9262 Acoustic and Vibration Measurements Page 1 of 2 AVCERT10 Rev. 1.3 15.05.18

CERTIFICATE NO.: SLM 25410 & FILT 5368

The performance characteristics listed below were tested. The tests are based on the relevant clauses of IEC 61672-3:2013

Tests Performed:	Clause	Result
Absolute Calibration	10	Pass
Acoustical Frequency Weighting	12	Pass
Self Generated Noise	11.1	Entered
Electrical Noise	11.2	Entered
Long Term Stability	15	Pass
Electrical Frequency Weightings	13	Pass
Frequency and Time Weightings	14	Pass
Reference Level Linearity	16	Pass
Range Level Linearity	17	NA
Toneburst	18	Pass
Peak C Sound Level	19	Pass
Overload Indicator	20	Pass
High Level Stability	21	Pass

Statement of Compliance: The sound level meter submitted for testing has successfully completed the class 1 periodic tests of IEC 61672-3:2013, for the environmental conditions under which the tests were performed. As public evidence was available, from an independent organization responsible for approving the results of pattern evaluation tests performed in accordance with IEC 61672-2:2013, to demonstrate that the model of sound level meter fully conformed to the requirements in IEC 61672-1:2013, the sound level meter submitted for testing conforms to the class 1 requirements of IEC61672-1:2013. A full technical report is available if required.

This Sound Level Meter included an Octave Filter Set. Tests were based on IEC 1260: 1995 and AS/NZS 4476 - 1997 and were conducted to test the following performance characteristics:

1. Relative attenuation

clause 5.3

Date of Calibration: 21/08/2019 Checked by:

Issue Date:

21/08/2019

Accredited for compliance with ISO/IEC 17025 - Calibration The results of the tests, calibration and/or measurements included in this document are traceable to Australian/national standards.



Accredited Lab. No. 9262 Acoustic and Vibration Measurements



Page 2 of 2 End of Calibration Certificate AVCERT10

CERTIFICATE OF CALIBRATION

CERTIFICATE NO: C28769

EQUIPMENT TESTED: Sound Level Calibrator

Manufacturer: Type No: **Owner:**

B&K 4230 Serial No: 1276091 EMM Consulting

Level 3, 175 Scott Street Newcastle, NSW 2300

Tests Performed: Measured output pressure level was found to be:

Parameter	Pre-Adj	Adj Y/N	Output: (db re 20 µPa)	Frequency: (Hz)	THD&N (%)
Level 1:	NA	N	93.83	996.49	1.41
Level 2:	NA	N	NA	NA	NA
Uncertainty:			±0.11 dB	±0.05%	±0.20 %
Uncertainty (at 9	5% c.l.) k=2				

CONDITIONS OF TEST:

Ambient Pressure: 994 hPa ±1.5 hPa Relative Humidity: 59 % ±5% **Temperature:** 23 °C ±2° C

Date of Calibration: 05/02/2021

Issue Date: 08/02/2021

Acu-Vib Test Procedure: AVP02 (Calibrators)

Test Method: AS IEC 60942 - 2017

Accredited for compliance with ISO/IEC 17025 - Calibration

Results of the tests, calibration and/or measurements included in this document are traceable to SI units through reference equipment that has been calibrated by the Australian National Measurement Institute or other NATA accredited laboratories demonstrating traceability.

The uncertainties quoted are calculated in accordance with the methods of the ISO Guide to the Uncertainty of Measurement and quoted at a coverage factor of 2 with a confidence interval of approximately 95%.



Accredited Lab. 9262 Acoustic and Vibration Measurements



HEAD OFFICE Unit 14, 22 Hudson Ave. Castle Hill NSW 2154 Tel: (02) 96808133 Fax: (02)96808233 Mobile: 0413 809806 Web site: www.acu-vib.com.au

Page 1 of 2 AVCERT02 Rev.1.6 25.08.20

	A SIGNIN	Notes 1			STREET, STREET	
	NUT D	NIT IV	I D NU	THE NU	SUT N/	
		ENES .				
		-				
		CFF				
			ALIBRATION			
		C	ALIBRATION	N		
			TIFICATE NO: C305			
EQU	IPMENT TEST	TED: S	ound Level Calibra	itor		
Man	ufacturer:					
	Type No:		Serial No:	79952		
	Owner:		Scott Street			
		Newcas	tle, NSW 2300			
	erformed:	Measure	d Output Pressure le	vel, Frequency &	Distortion	
<u> </u>	omments:	See Deta	ails overleaf. All Test	Passed.		
Parame	ter Pre-	Adj Y/N	Output: (dB re 20 µPa)	Frequency	THD&N	
Level		N	94,12 dB	(Hz) 999.99 Hz	(%) 1.58 %	
Level	2: NA	N	114.05 dB	999.99 Hz	1.12 %	
	Uncertainty		±0.11 dB	±0.05%	±0.20 %	
	ty (at 95% c.l.) ON OF TEST:) k=2				
	nt Pressure	1007 hl			16/09/2021	
	emperature e Humidity		C ±1° C Date of 5 ±5%		16/09/2021 16/09/2021	
Relative	enumunty	45 70	1070	Date of issue .	10/09/2021	
Acu	I-Vib Test					
Р	rocedure:	Test Met	hod: AS IEC 60942 -	- 2017	/	
Снеск	KED BY:	K)	AUTHORISED	St		
Снеск	KED BY: .	R	AUTHORISED SIGNATURE:		500	
	Accr		SIGNATURE:	25 - Calibration		
Results	Accr of the tests, calibra eference equipment	ation and/or int that has b	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in th even calibrated by the Austra	Hein Rein 25 - Calibration is document are traceal lian National Measurem	ble to SI units	
Results of through re	Accr of the tests, calibra eference equipmen other	ation and/or in that has b NATA accre	SIGNATURE:	Hein 25 - Calibration his document are traceal lian National Measurem ating traceability.	ble to SI units ent Institute or	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmei other is report applies of tainties quoted are	ation and/or Int that has b NATA accre Inly to the iter calculated i	SIGNATURE: ompliance with ISO/IEC 1700 measurements included in th been calibrated by the Austra edited laboratories demonstra m identified in the report and in accordance with the method	Action 25 - Calibration his document are traceal lian National Measurem ating traceability. may not be reproduced bods of the ISO Guide to	ble to SI units ent Institute or in part. the Uncertainty	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmei other is report applies of tainties quoted are	ation and/or Int that has b NATA accre Inly to the iter calculated i	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in th even calibrated by the Austra edited laboratories demonstra m identified in the report and	Action 25 - Calibration his document are traceal lian National Measurem ating traceability. may not be reproduced bods of the ISO Guide to	ble to SI units ent Institute or in part. the Uncertainty	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmei other is report applies of tainties quoted are	ation and/or Int that has b NATA accre Inly to the iter calculated i	SIGNATURE: ompliance with ISO/IEC 1700 measurements included in th been calibrated by the Austra edited laboratories demonstra m identified in the report and in accordance with the method	Action 25 - Calibration his document are traceal lian National Measurem ating traceability. may not be reproduced bods of the ISO Guide to	ble to SI units ent Institute or in part. the Uncertainty	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmei other is report applies of tainties quoted are	ation and/or nt that has b NATA accre nly to the iter e calculated i led at a cove	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in th veen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the method erage factor of 2 with a confid	<i>Hein</i> 25 - Calibration his document are traceal lian National Measurem ating traceability. may not be reproduced ods of the ISO Guide to lence interval of approxi	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmei other is report applies of tainties quoted are	ation and/or nt that has b NATA accre nly to the iter e calculated i led at a cove	SIGNATURE: ompliance with ISO/IEC 1700 measurements included in th been calibrated by the Austra edited laboratories demonstra m identified in the report and in accordance with the method	<i>Hein</i> 25 - Calibration his document are traceal lian National Measurem ating traceability. may not be reproduced ods of the ISO Guide to lence interval of approxi	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot	ation and/or in that has b NATA accree haly to the iten e calculated i led at a cove	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in th veen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the method erage factor of 2 with a confid	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. Imay not be reproduced ods of the ISO Guide to thence interval of approxite ectronic	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot surement and quot workLD RECOGNIBED CCREDITATION	ation and/or in that has b NATA accree only to the iten the calculated in the d at a cover CALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the included in the redited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confident CU-VIDELE IBRATIONS SALES	Action 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced bods of the ISO Guide to tence interval of approxi ecctronic RENTALS REPAI	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the readilted laboratories demonstra m identified in the report and in accordance with the methor erage factor of 2 with a confid CU-VIDELE IBRATIONS SALES ad Office & Calibration Laboo E 14, 22 Hudson Ave. Castle HUNS	Action Action	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the seen calibrated by the Austra edited laboratories demonstra m identified in the report and in accordance with the method arage factor of 2 with a confid U - VID ELE IBRATIONS SALES ad Office & Calibration Labo	Action Action	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the sedited laboratories demonstration in identified in the report and in accordance with the method arage factor of 2 with a confident CU-VibEle IBRATIONS SALES ad Office & Calibration Laboo rt 14, 22 Hudson Ave. Castle Hill NSY (02) 9680 8133 WWW, acu-vib.com.au	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration construction constr	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration worLD Recognised accretorration accretorrati	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	N91
Results of through ro Th The uncer of Meas	Accr of the tests, calibra eference equipmen other is report applies or tainties quoted are surement and quot worLD Recognised accretorration worLD Recognised accretorration accretorrati	Ation and/or in that has b NATA accree hay to the iter e calculated i led at a cover ACALI	SIGNATURE: ompliance with ISO/IEC 1702 measurements included in the reen calibrated by the Austra addited laboratories demonstra m identified in the report and in accordance with the methor arage factor of 2 with a confid CU-VIDEE IBRATIONS SALES ad Office & Calibration Laboo r 14, 22 Hudson Ave. Castle Hill NS' (02) 9680 8133 WWW.acu-vib.com.au Bge 1 of 2 Calibration Certificato	Active 25 - Calibration his document are traceal lian National Measurem ating traceability. I may not be reproduced ods of the ISO Guide to tence interval of approxi- tence interval of approxi- RENTALS REPAI atory w 2154	ole to SI units ent Institute or in part. the Uncertainty mately 95%.	

			ALIBRATION		
			TIFICATE NO: C308		
		TED: S	ound Level Calibra	tor	
Manufact		Svantek		00211	
		SV-36	Serial No: onsulting	86311	
Ū,			, 20 Chandos St		
	5	St Leona	ards NSW 2065		
Tests Perfor			d Output Pressure le		Distortion
Comm			ails overleaf. All Test		TUDAN
Parameter	Pre- Adi	Adj Y/N	Output:	Frequency (Hz)	THD&N (%)
Level1:	NA	T/N N	(dB re 20 μPa) 94.05 dB	999.99 Hz	1.00 %
Level2:	NA	N	114.05 dB	999.99 Hz	1.00 %
	rtainty		±0.11 dB	±0.05%	±0.20 %
Uncertainty (at 9		k=2			
CONDITION OF Ambient Pres		1002 6	Pa±1hPa D	ate of Receipt :	20/10/2021
Tempera				are or receipter .	20/10/2021
Relative Hum			±5%	Date of Issue :	20/10/2021
Acu-Vib Proced			Calibrators) hod: AS IEC 60942 -	2017 hM	Δ
Proced CHECKED BY Results of the te	Accre sts, calibrat e equipmen	Fest Meth		Jack Jack 25 - Calibration is document are tracea ian National Measurem	
Proced CHECKED BY Results of the ter through reference This report The uncertainties	Accre sts, calibrat e equipmen other t t applies on quoted are	edited for co tion and/or r at that has be NATA accre ly to the iter calculated i	hod: AS IEC 60942 - AUTHORISED SIGNATURE: measurements included in th een calibrated by the Austral	Jack 5 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to	ble to SI units ent Institute or I in part. the Uncertainty
Proced CHECKED BY Results of the ter through reference This report The uncertainties	Accre sts, calibrat e equipmen other t t applies on quoted are	edited for co tion and/or r at that has be NATA accre ly to the iter calculated i	hod: AS IEC 60942 - AUTHORISED SIGNATURE: measurements included in the een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the method	Jack 5 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to	ble to SI units ent Institute or I in part. the Uncertainty
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipmen other t t applies on quoted are	Fest Meth edited for co tion and/or r at that has b NATA accre hy to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid	Jack 25 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n it that has be NATA accre hy to the iter calculated i ed at a cove	AUTHORISED SIGNATURE: measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid	Jack 5 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measurement	Accre sts, calibral e equipmen other N t applies on quoted are tt and quote	edited for co tion and/or n it that has be NATA accre hy to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid	Jack 5 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipmen other h a applies on quoted are at and quote	edited for continue and/or nation and/or nation and/or nation and/or nation and/or nation and/or national and and a second	AUTHORISED SIGNATURE: measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid	Jack 25 - Calibration is document are tracea ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi Pectronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n that has b NATA accre ly to the iter calculated i ed at a cove	AUTHORISED SIGNATURE: mpliance with ISO/IEC 1702 measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid March Control Confidence BRATIONS SALES and Office & Calibration Laboo 14, 22 Hudion Ave. Castle Hill NST (2) 9660 813	Jack 5 - Calibration is document are traceal ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi ecctronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n that has b NATA accre ly to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: mpliance with ISO/IEC 1702 measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid BRATIONS SALES d Office & Calibration Labo (02) 9680 8133 www.acu-vib.com.au ge 1 of 2 Calibration Certificate	Jack 5 - Calibration is document are traceal ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi ecctronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n that has b NATA accre ly to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: mpliance with ISO/IEC 1702 measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid BRATIONS SALES d Office & Calibration Labo (02) 9680 8133 www.acu-vib.com.au ge 1 of 2 Calibration Certificate	Jack 5 - Calibration is document are traceal ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi ecctronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n that has b NATA accre ly to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: mpliance with ISO/IEC 1702 measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid Marconace with the methor rage factor of 2 with a confid BRATIONS SALES d Office & Calibration Labo (02) 9680 8133 www.acu-vib.com.au ge 1 of 2 Calibration Certificate	Jack 5 - Calibration is document are traceal ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi ecctronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.
Proced CHECKED BY Results of the ter through reference This report The uncertainties of Measuremen	Accre sts, calibrat e equipment other h t applies on quoted are at and quote	edited for co tion and/or n that has b NATA accre ly to the iter calculated i ed at a cove	hod: AS IEC 60942 - AUTHORISED SIGNATURE: mpliance with ISO/IEC 1702 measurements included in th een calibrated by the Austral dited laboratories demonstra m identified in the report and in accordance with the methor rage factor of 2 with a confid Marcona autor CU-VIDEE BRATIONS SALES ad Office & Calibration Laboo 14, 22 Hudion Ave. Castle Hill NS' (02) 9680 8133 www.acu-vib.com au ge 1 of 2 Calibration Certificate	Jack 5 - Calibration is document are traceal ian National Measurem ting traceability. may not be reproduced ods of the ISO Guide to ence interval of approxi ecctronic RENTALS REPAI	ble to SI units ent Institute or I in part. the Uncertainty mately 95%.

1/18

\//

N//

1

